

## APPLICATION NOTE

### Online Monitoring of Caustic and Carbonate Using a ClearView® db Photometer

#### Purpose

To simultaneously measure caustic (NaOH) and sodium carbonate in aqueous process streams, particularly at low (<2%) caustic concentrations, using our GUIDED WAVE™ ClearView® db Dual-Beam Photometer and fiber optic probe.

#### Measurement Background

The dominance of water in the NIR hampers the measurement of caustic. Nevertheless, there are several successful reports of using full-spectrum FT-NIRs and discrete wavelength photometers for moderate caustic concentrations. Watson and Baughman (Spectroscopy, 2(1) 44-48 (1984)) summarized a typical approach using the spectral region from 1700 to 2300 nm and narrow optical cells of <1 mm. Their calibration (Figure 1) is a caustic calibration used when other species are present, such as carbonate and Na<sub>2</sub>S. Our lower range of interest is circled on their calibration.

#### Approach

We used the same procedure as described in our article (Spectroscopy, 15 (2) 40-46 (2000)). Samples were thermostated in a sample cell at 35 °C and analyzed with our spectrometer. A partial least squares (PLS) analysis of the spectral calibration set was performed. This analysis revealed that several analyzing wavelengths were required in addition to a reference wavelength for both measurements. A ClearView db photometer was configured with those wavelengths. The samples were re-run in the ClearView db and their absorbances were recorded. Multiple linear regression (MLR) coefficients were then calculated.

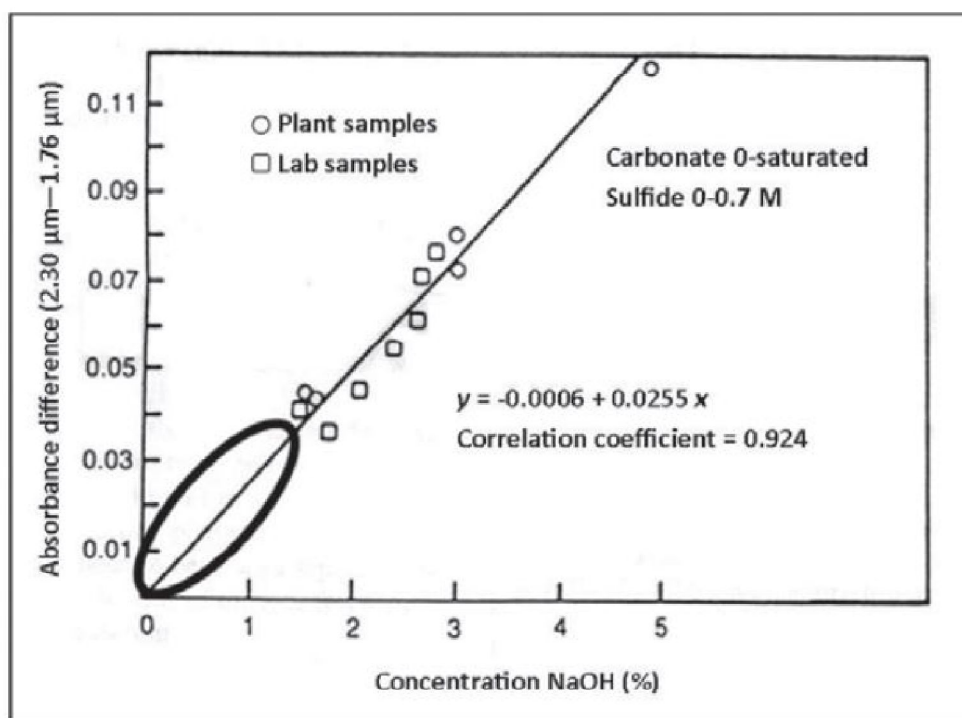


Figure 1: Plot of absorbance difference at 2.30 and 1.76  $\mu\text{m}$  versus percent of equivalent NaOH. Samples contained NaOH,  $\text{Na}_2\text{CO}_3$ , and  $\text{Na}_2\text{S}$ , %NaOH calculated assuming  $\text{Na}_2\text{S}$  was hydrolyzed.

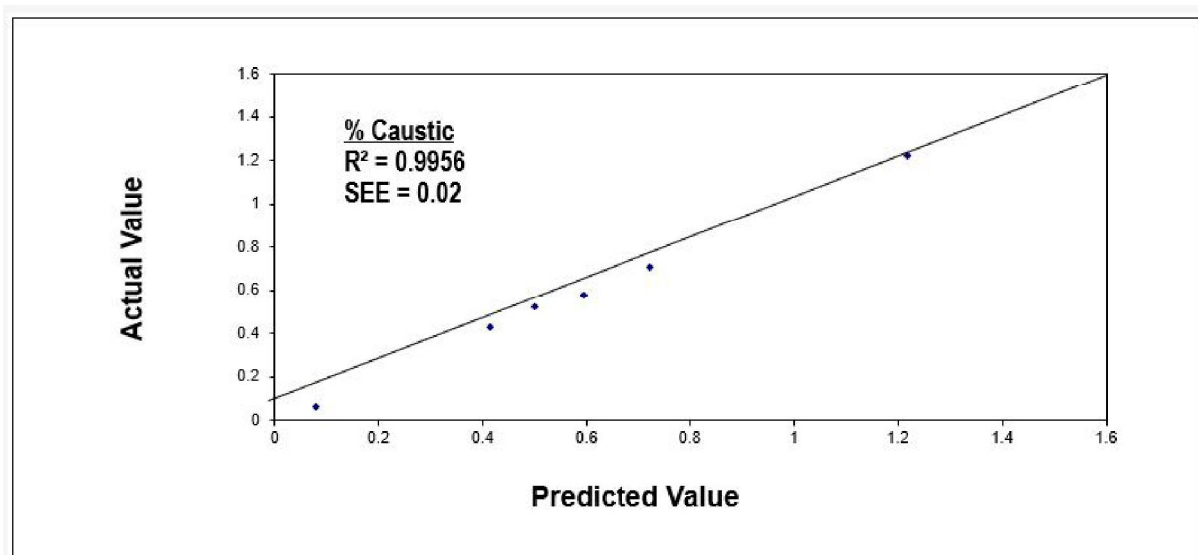


Figure 2: Accuracy chart for Caustic determination by NIR.

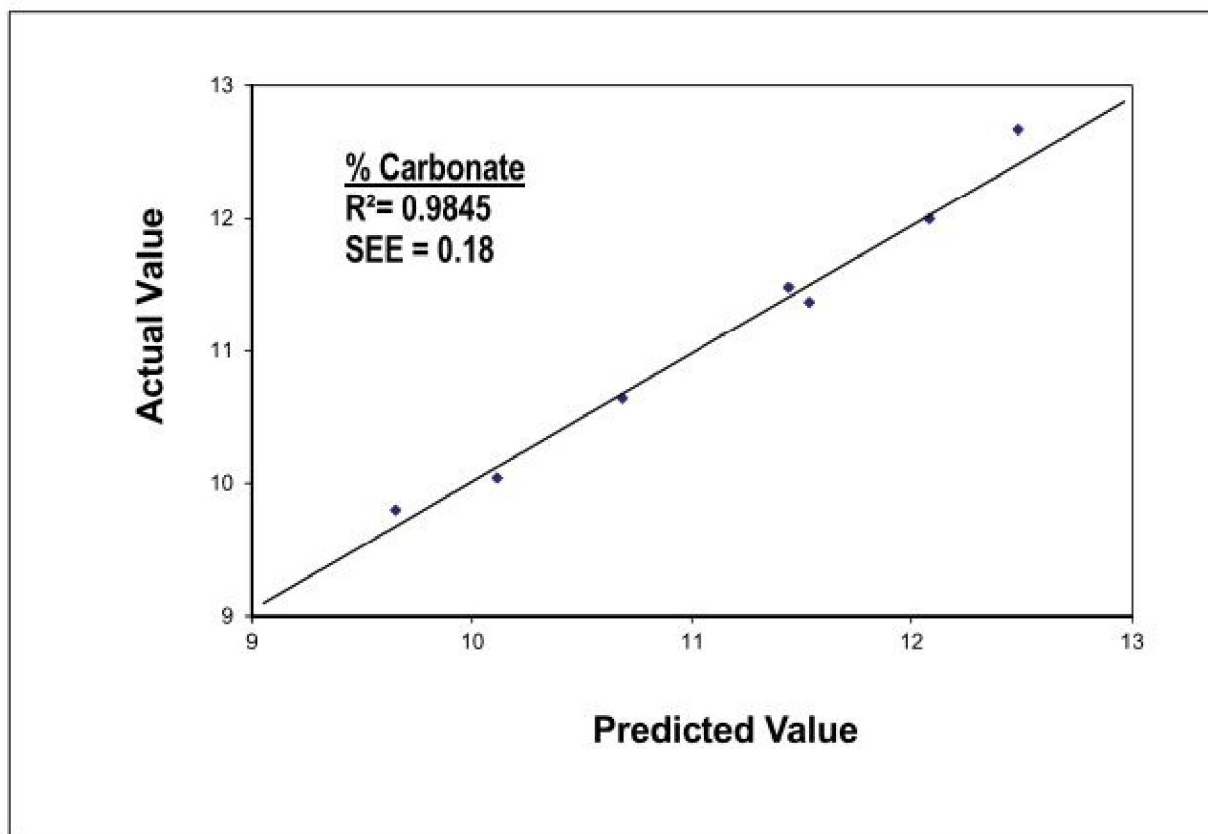


Figure 3: Accuracy chart for Carbonate determination by NIR.

## Results

The resulting MLR calibrations are shown in Figure 1 and 2. Months of on-line data have demonstrated the linearity of the caustic calibration with a precision of better than  $\pm 0.1$ . We have extended this approach to another customer's sample set in the 1-10% caustic range with an  $R^2=0.9938$  and an SEE of  $\pm 0.47$ . It is pointed out that temperature conditioning of the sample in the slip stream to better than  $2^\circ\text{C}$  is important, primarily for caustic. The ClearView db has the capability to correct the calibration for wider temperature fluctuations using the measured sample temperature from an RTD sensor. Nevertheless, this places demands on the sampling system containing the fiber optic probe. Due to the likely need of cleaning the sapphire windows in the probe with HCl, we recommend a probe with a Hastelloy® B body for concentrations over 20%, titanium for concentrations 60-80%, and Kalrez® 6375 wetted o-ring seals.

## Conclusion

Our multiple wavelength ClearView db photometer has the sensitivity and stability to measure low levels of caustic in the presence of carbonate. This has been successfully demonstrated online. For more detailed information regarding system specifications and the ClearView db photometer please contact a Process Insights sales or technical specialist.

## GAIN REAL-TIME INSIGHT INTO YOUR PROCESS

Process Insights manufactures and delivers premium sensors, monitors, detectors, analyzers, instrumentation, and software that are mission-critical to keep your operations, personnel, and the environment safe – every day across the globe.

Get the most reliable, precision analytical technologies available on the market today. We will work to match your needs and budget, and provide the optimal, and most stable process analysis solution for your application.

---

## CENTERS OF EXCELLENCE | PROVIDING PROVEN SOLUTIONS

Process Insights is committed to solving our customers' most complex analytical, process, and measurement challenges everyday.

### Process Insights – The Americas

4140 World Houston Parkway Suite 180, Houston, TX 77032, USA +1 713 947 9591

### Process Insights – EMEA

ATRICOM, Lyoner Strasse 15, 60528 Frankfurt, Germany +49 69 20436910

### Process Insights – APAC

Wujiang Economic and Technology, Development Zone, No. 258 Yi He Road, 215200 Suzhou, Jiangsu Province, China +86 400 086 0106

---

For a complete range of products, applications, systems, and service options, please contact us at: [info@process-insights.com](mailto:info@process-insights.com)

For a complete list of sales & manufacturing sites, please visit:  
<https://www.process-insights.com/about-us/locations/>

COSA Xentaur, Tiger Optics, Extrel, Alpha Omega Instruments, ATOM Instrument, MBW Calibration, MGA, Guided Wave, ANALECT and LAR TOC Leader are trademarks of Process Insights, Inc.



REVOLUTIONIZING MEASUREMENT

**EVERYWHERE**